



COLOR LCD AND MONOCHROME LCD CONTRAST DISPLAYS OF RADIOLOGY MEDICAL

Dr Iqra Sultan^{1*}, Dr. Ayesha Maheen², Dr. Aida Naz³, Shaher Bano⁴, Summya Gulzar⁵, Dr Aimen Shabbir⁶, Dr Andleeb Iqbal⁷, Dr Fahmida Khaton⁸, Kashif Lodhi⁹

ABSTRACT:

In symptomatic radiology, monochrome presentations for clinical evaluation are normally suggested because of their higher luminance. Standard shaded displays can be used as another less expensive option, but they have a lower luminance. The purpose of the current review was to consider image quality for both types of presentations. Images of a contrast ghost from the CDRAD were examined by four radiologists using a 2 megapixel (143 discs/m² of extreme luminance) shading showcase as well as 2 Mp (295 compact discs/m²) and 3 Mp monochrome presentations. Thirty lumbar spine x-rays were also examined by four radiologists using shading and 2-MP monochrome presentation as part of a visual examination. Tiny contrasts were found between the cases when reading the CDRAD images. The VGA scores were j0.29 for shading and j0.25 for the monochrome presentation (p=0.26; NS). It thus seems conceivable to use shading shows in symptomatic radiology, given that the change of grey scale is used.

Keywords: Color LCD, Monochrome LCD, Contrast Displays.

¹*CMH Muzaffarbad, sultaniqra64@gmail.com

²MH Rawalpindi, ayesha_maheen65@live.com

³DHQ Mirpur, aidanaz.12345@gmail.com

⁴CMH Rawalakot AJK, khanshyri@gmail.com

⁵CMH Rawalakot ajk, azhirbutt33@gmail.com

⁶CMH Muzaffarabad, aimenshabbir11@gmail.com

⁷Consultant Radiologist, Rawal Institute of Health Sciences, annieiqbal99@gmail.com

⁸Associate professor, Department of Biochemistry, College of Medicine

University of Hail, KSA, f.khaton@uoh.edu.sa

⁹Department of Agricultural, Food and Environmental Sciences. Università Politénica delle Marche Via Brece Bianche 10, 60131 Ancona (AN) Italy, k.lodhi@studenti.unibg.it

***Corresponding Author:** - Dr Iqra Sultan

*CMH Muzaffarbad, sultaniqra64@gmail.com

DOI: 10.53555/ecb/2023.12.Si13.262

INTRODUCTION:


Numerous points of concern in visual radiology are analyzed with film-based radiology. Firstly, the technologies used by the film can now be separated into four distinct developments: the acquisition of material, the planning of the image, the storing of material and the presentation [1]. Could of these methods can and should be independently progressed. In the following four stages, the data in the advanced image will be transferred to the viewer, usually as light and shaded versions [2]. It is important that high-quality displays all together should not compromise the current advances in the framing of images. In the prose, monochrome clinical evaluations are usually recommended because of their greater luminance. The biggest drawback to monochrome screens is that they cost a lot and have driven a few organizations to use regular shading shows that are much more economical because they are manufactured in bulk for the entire PC industry. Since late, a trend has been formed from shows which rely on cathode beam tubes to levels based on fluid gem shows. This is upheld by a few studies [11-40]. We decided to test the unfounded hypothesis that in a certain picture quality element no difference is noticeable between contrast-detailed fantastic pictures in a buyer grade LCD display and a monochrome LCD clinical appraisal of a similar intent [3-4]. We too decided to test the unfounded hypothesis that a significant difference between clinical radiogram of the lumbar spine on similar screens was not made in the symptomatic quality of the picture [5].

METHODOLOGY:

The review considered three kinds of showcases. The main correlation was made between a 20-inch LCD (2000 FP Ultra Sharp, Dell, Round Rock, TX, USA) with a lens of 1,300 and 1,700 pixels, 2 megapixels (MP), and a 20-inch monochrome LCD (MFGD 2320, Barco, Kortrijk, Belgium) with a lens of 1,200,1,600 pixels, 2 MP. Some tests were also performed using a 20-inch monochrome LCD (MFGD 3220 D, Barco) with a lens of 2,537,049 pixels, 3 MP. All examinations were associated

with a PACS workstation using a web interface (Centricity Enterprise Web v2.1, GE Medical Systems) for image multiplication. The monochrome display cases were adjusted between 1 and 300 cd/m² according to section 14 of the DICOM (Computerized Imaging and Interchanges in Medication) standard on grayscale, using the implicit photometer (I-monitor) and the programming of Medical Pro. The 2 Mp program was not celebrated as an adjustment would require additional programming on an approved PACS clinical workstation. Each of the three shows was performed with a luminance meter spot (Minolta LS-100, Minolta Co. Ltd., Osaka, Japan) and AAPM TG-18 test targets. As the estimation deviation was approximately 1 m, the surrounding light was systematically taken into account for each estimation. Ambient light settings were estimated using a luxmeter. The 2-MP shading show had a basic luminance of 0.87 discs/m² and an extreme luminance of 148 discs/m². The 2-MP monochrome show had a basic luminance of 1.58 discs/m² also, an extreme luminance of 295 compact discs/m², all qualities estimated at 23 lx of illumination. The cost of the showcases when they were created in 2003/2004 was approximately \$2,400 for the shading show, \$15,000 for the 2-MP monochrome show and \$17,000 for the 3-MP show. The costs have decreased significantly since the company's inception, but the report is comparative. Two types of examinations were performed: one using a difference detail phantom and the other using clinical X-rays of the lumbar spine. Correlation using the appearance of difference detail: Images of the appearance of a CDRAD 2.0 difference detail were seen on all presentations. The appearance consists of a 26626712 mm polymathic methacrylate sheet with apertures of distinct depth and width. Using this apparition, a four-choice constraining decision is made, the objective being to distinguish the same number of foci as is conceivable. All localization results have been modified according to the CDRAD phantom customer manual.

Figure 1:

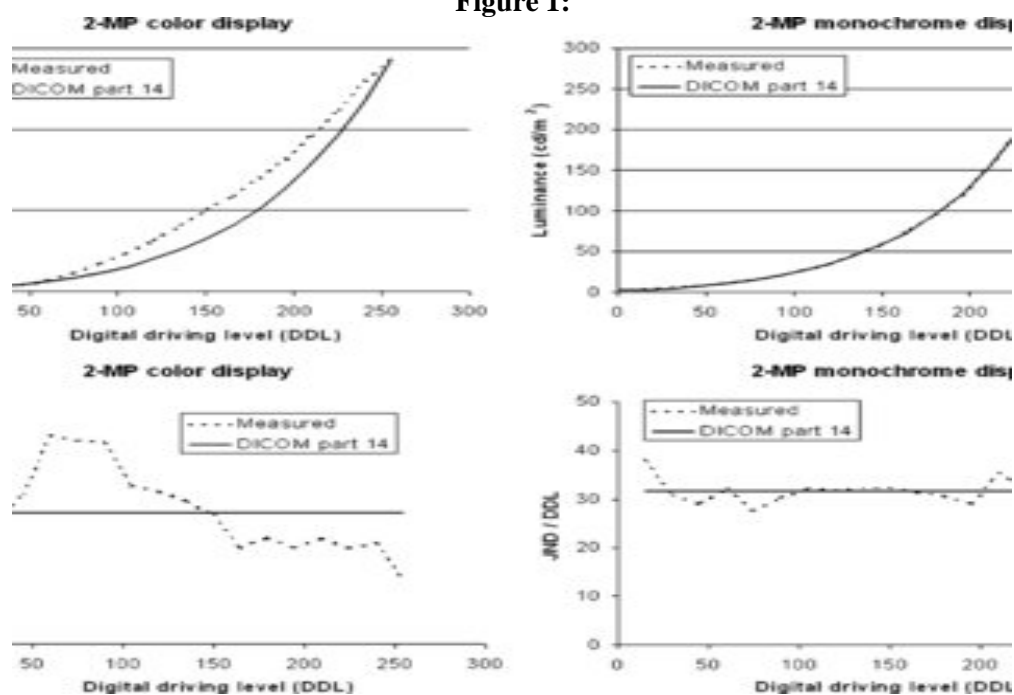**RESULTS:**

The fitting curves for 2-MP shading and 2-MP monochrome presentations are shown in Figure 1. The correlations between shading and monochrome presentations with various high-contrast phantom images and surrounding illumination levels are shown in Figure 2. Using a flat panel image with low illumination, the average image quality (IQF) was 40 for 2-MP shading and 43 for the monochrome 2-MP presentation. At high illumination, the comparative IQF values were 45 and 43. When the phosphor plate image was

modified, the IQF values were increased to 53 and 54, demonstrating poor image quality, with still exceptionally low contrast between the two presentations. While the monochrome exposure was exchanged for a 3-MP unit with no zoom allowed, the IQF estimates were 45 for the 2-MP shading and 42 for the 3-MP monochrome exposure. The VGA of the clinical pictures provided very little contrast between the two types of presentation; furthermore, there was no huge distinction for the overall score (Table 1).


Table 1:

Criterion (according to [4])	Visual Grading Analysis Score (VGAS)			
	2-MP Color	2-MP Monochrome	Difference	<i>p</i> value
Visually sharp reproduction, as a single line, of the upper- and lower-plate surfaces in the centered beam area	-0.13	-0.23	0.09	0.13
Visually sharp reproduction of the pedicles	-0.32	-0.19	-0.13	0.03*
Reproduction of the intervertebral joints	-0.58	-0.45	-0.13	0.01*
Reproduction of the spinous and transverse processes	-0.15	-0.28	0.13	0.03*
Visually sharp reproduction of the cortex and trabecular structures	-0.17	-0.09	-0.08	0.15
Reproduction of the adjacent soft tissues, particularly the psoas shadows	-0.41	-0.42	0.01	0.89
Reproduction of the sacro-iliac joints	-0.18	-0.07	-0.11	0.07
Overall score	-0.28	-0.25	-0.03	0.24

Positive scores mean higher image quality than the reference image, negative scores lower.

* = Significant at the 0.05 level.

Figure 2:

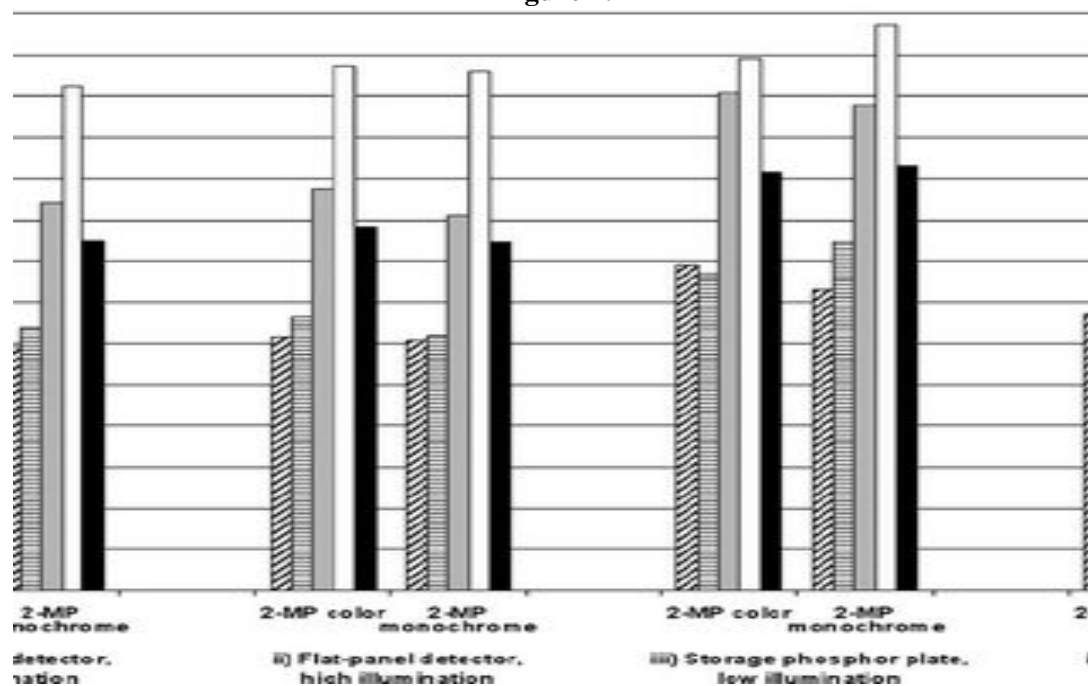

DISCUSSION:

This test showed no vital image quality discrepancy between a typical 2-MP LCD shading display and the 2-MP monochrome LCD clinical assessment display, not using the contrast information presentation nor visual inspection [6]. As seen in the range of clinical tests such as CT-RC,5 x-ray of wrist fractures, automated radiographs of the patients presenting rheumatoid Arthritis early on, and chest x-rays of interstitial lung disease, we find few studies that have demonstrated comparable exposures for shading. In another analysis, Goo et al observed that the luminance of the chest X-rays was satisfactory as low as 86 cd / m². The principle reason for adjusting a screen as indicated by DICOM section 15 is to acquire comparable picture introduction on all showcases [7]. An alignment conveys the all-out differentiation of the showcase similarly over the whole grayscale and articles will subsequently be given a similar difference paying little heed to regardless of whether they are available in brilliant or dim pieces of the picture. At the point when the undertaking is to discover known articles in a picture, for example, focuses in a difference detail apparition, the window/level controls can be utilized to upgrade picture contrast [8]. The differential qualities of the showcase have been seen to be less important, and the clamor characteristics of the locator and the clamor from the image display become more significant [9]. However, it does not mean that it is easy to coordinate a display. Medical portraits are not so similar to images that display a contrast detail such that the anatomy can often be found such glorious or bland snapshots. A positive presentation of

images is even more important if, for example, a present image is studied on another monitor in the past. The picture source and not the exhibits should make some difference between the images [10].

CONCLUSION:

In summary, there was no visible difference in image quality between a monochrome LCD monitor of medical grade and an LCD shading with the same spatial target nor a ghost of difference information or a visual assessment of the full potential when a grayscale adjustment was used.

REFERENCES:

1. Samei E, Badano A, Chakraborty D, Compton K, Cornelius C, Corrigan K, Flynn MJ, Hemminger B, Hangiandreou N, Johnson J, Moxley M, Pavlicek W, Roehrig H, Rutz L, Shepard J, Uzenoff R, Wang J, Willis C: Assessment of Display Performance for Medical Imaging Systems, Report of the American Association of Physicists in Medicine (AAPM) Task Group 18. AAPM online report No. 03. April, Medical Physics Publishing, Madison, WI, 2015
2. Krupinski E, Roehrig H, Furukawa T: Influence of film and monitor display luminance on observer performance and visual search. *Acad Radiol* 6:411Y418, 2017
3. Krupinski EA, Roehrig H: Pulmonary nodule detection and visual search: P45 and P104 monochrome versus color monitor displays. *Acad Radiol* 9:638Y645, 2018
4. Geijer H, Beckman K-W, Andersson T, Persliden J: Image quality vs radiation dose for

- a flat-panel amorphous silicon detector: a phantom study. *Eur Radiol* 11:1704Y1709, 2017
5. Chakrabarti K, Kaczmarek RV, Thomas JA, Romanyukha A: Effect of room illuminance on monitor black level luminance and monitor calibration. *J Digit Imaging* 16: 350Y355, 2013
 6. Ikeda M, Ishigaki T, Shimamoto K, Kodera Y, Koyama S, Usami H, Kato K: Influence of monitor luminance change on observer performance for detection of abnormalities depicted on chest radiographs. *Invest Radiol* 38:57Y63, 2013
 7. Wang J, Compton K, Peng Q: Proposal of a quality index or metric for soft copy display systems: contrast sensitivity study. *J Digit Imaging* 16:185Y202, 2017
 8. Peer S, Giacomuzzi SM, Peer R, Gassner E, Steingruber I, Jaschke W: Resolution requirements for monitor viewing of digital flat-panel detector radiographs: a contrast detail analysis. *Eur Radiol* 13:413Y417, 2003
 9. Hangiandreou NJ, Fetterly KA, Felmler JP: Optimization of a contrast-detail-based method for electronic image display quality evaluation. *J Digit Imaging* 12:60Y67, 1999
 10. Van Metter R, Zhao BS, Kohm K: The sensitivity of visual targets for display quality assessment. *Proc SPIE* 3658:254Y268, 2018.
 11. Khan MI, Ashfaq F, Alsayegh AA, Hamouda A, Khatoon F, Altamimi TN, et al. Advanced glycation end product signaling and metabolic complications: Dietary approach. *World Journal of Diabetes* [Internet]. 2023 Jul 15;14(7):995–1012. Available from: <http://dx.doi.org/10.4239/wjd.v14.i7.995>
 12. Aladel A, Khatoon F, Khan MI, Alsheweir A, Almutairi MG, Almutairi SO, et al. Evaluation of miRNA-143 and miRNA-145 Expression and Their Association with Vitamin-D Status Among Obese and Non-Obese Type-2 Diabetic Patients. *Journal of Multidisciplinary Healthcare* [Internet]. 2022 Dec; Volume 15:2979–90. Available from: <http://dx.doi.org/10.2147/jmdh.s391996>
 13. Kumar R, Khan MI, Ashfaq F, Alsayegh AA, Khatoon F, Altamimi TN, et al. Hesperidin Supplementation Improves Altered PON -1, LDL Oxidation, Inflammatory Response and Hepatic Function in an Experimental Rat Model of Hyperlipidemia. *Indian Journal of Clinical Biochemistry* [Internet]. 2023 Jun 20; Available from: <http://dx.doi.org/10.1007/s12291-023-01140-5>
 14. Ashfaq F, Aljaadi AM, Salaka AS, Noorwali EA, Khatoon F, Khan MI. Comparison of TCN-2 (776C>G) Gene Polymorphism and Vitamin B12 Status with Different Body Mass Index among Saudi Adults. *Life* [Internet]. 2023 May 15;13(5):1185. Available from: <http://dx.doi.org/10.3390/life13051185>
 15. Mughal h, Abdullah m, Jamil a, Malik a, Rasheed s, Khatoon f. Efficacy of methotrexate alone or with low-dose prednisone in alopecia areata totalis. *Biological and Clinical Sciences Research Journal* [Internet]. 2023 Jun 23;2023(1):332. Available from: <http://dx.doi.org/10.54112/bcsrj.v2023i1.332>
 16. SIDDIQUI E, ABBASI M, KHOSA M, MOHSIN R, JABEEN N, SIDDIQUE U, et al. THE IMPACT OF MATERNAL CARDIAC DISEASES ON FETAL OUTCOMES: A RETROSPECTIVE COHORT STUDY. *Biological and Clinical Sciences Research Journal* [Internet]. 2023 Jun 16;2023(1):315. Available from: <http://dx.doi.org/10.54112/bcsrj.v2023i1.315>
 17. Altamimi T, Balouch F. Mini Review; Role of Changes in SARS-CoV-2 Spike Protein and Its Human Interaction. *Egyptian Academic Journal of Biological Sciences C, Physiology and Molecular Biology* [Internet]. 2023 Jun 9;15(1):503–7. Available from: <http://dx.doi.org/10.21608/eajbsc.2023.303781>
 18. Ali S, Saeed SJ, Zahid S, Rashid I, Khatoon F, Altamimi TN. Impact of Evaluation of Tumour Grade by Core Needle Biopsy on Clinical Risk Assessment and Patient Selection for Adjuvant Systemic Treatment in Breast Cancer. *Pakistan Journal of Medical and Health Sciences* [Internet]. 2023 Mar 15;17(2):817–9. Available from: <http://dx.doi.org/10.53350/pjmhs2023172817>
 19. Khan MI, Hashmi MO, Abid SUH, Khan B, Iqbal H, Khatoon F. Mid-Term Clinical and Echocardiographic Outcomes of Percutaneous Transvenous Mitral Commissurotomy in Patients with Rheumatic Mitral Stenosis. *Pakistan Journal of Medical and Health Sciences* [Internet]. 2023 Mar 15;17(2):793–5. Available from: <http://dx.doi.org/10.53350/pjmhs2023172793>
 20. Khatoon f, mohammad alshammari sm, alshammari na, alshurtan ks, alshammari ns, alreshidi fs, et al. Perception, awareness and attitude towards varicose veins among employees working in prolonged sitting and standing postures in hail region, saudi arabia. *Medical science* [internet]. 2023 may 2;27(135):1–8. Available from: <http://dx.doi.org/10.54905/disssi/v27i135/e206ms2985>
 21. Khan m, nouman m, hashim h, latif s, husain s, sattar s, et al. A correlation biomarker between

- bmi and lipid peroxidation in type 2 diabetes mellitus with and without other complications. *Biological and clinical sciences research journal* [internet]. 2023 Apr 21;2023(1):253. Available from: <http://dx.doi.org/10.54112/bcsrj.v2023i1.253>
22. Sohair A M Shommo, Firas S. Azzeh, Alsolami Ahmed Khatoon F Et Al, Prevalence Of Serum Vitamin Deficiency In Pakistan Of Chronic Fatigue Without Any Systemic Illness 2023. Volume -12, Special Issue-13 (2023 Doi; 10.53555/Ecb/2023.12.Si13)
23. Ahmed S , Mahmood T , Mudasir M, Khatoon F et al. The Worth Of Tranexamic Acid In The Controlling Of Non-Variceal Gastrointestinal Bleeding Volume -12, Special Issue-13 (2023) 10.53555/ecb/2023.12.Si13.1982023.25/11/2023
24. Gul S, mir n, Fatima k, tahir s, Younis ns, Khatoon F, et al. Catheter-related infections in hemodialysis: frequency and microbiological profile patients undergoing antimicrobial lock therapy with gentamicin for prophylaxis. *Biological and Clinical Sciences Research Journal* [Internet]. 2023 Apr 18;2023(1):247. Available from: <http://dx.doi.org/10.54112/bcsrj.v2023i1.247>
25. Alreshidi FF, Alshammari RF, Alenazi SH, Alshammry TE, Altamimi TN, Almughais ES, et al. Sciatica pain in Saudi population: Knowledge and attitude towards sciatica pain and treatment methods among the population of Hail in Saudi Arabia. *Medical Science* [Internet]. 2023 Mar 1;27(133). Available from: <http://dx.doi.org/10.54905/disssi/v27i133/e142ms2906>
26. Zahra A, Hassan SU, Hassan MS, Parveen N, Park JH, Iqbal N, Khatoon F, Atteya MR. Effect of physical activity and sedentary sitting time on psychological quality of life of people with and without disabilities; A survey from Saudi Arabia. *Front Public Health*. 2022 Sep. fpubh.2022.998890 PMID: 36225781; PMCID: PMC9548647. <https://doi.org/10.3389/fpubh.2022.998890>
27. Almughais, E. S., Abdullah Alshammari, K. A., Alshammari, H. H., Alreshidi, F. F., Alarfaj, R., Alshammari, R. F., Altamimi, T. N., Aboras, R., Almeahmadi, S. A., & Balouch, F. K. (2023, February 5). "Assessment of knowledge and practice of Carpal tunnel syndrome among pregnant and non-pregnant women in Hail region, Saudi Arabia." *Medical Science*, 27(132), 1–8. <https://doi.org/10.54905/disssi/v27i132/ee116ms2910>
28. Khatoon, F., Alshammari, R. A., Batool, A., Elhaj, A. H., Alreshidi, F. F., Elhussein, G. E. M. O., Abdalla, R. A. H., Elhag, A. B. M., & Balouch, Z. (2022, October 30). Systematic Review on Implication for DNA Assisted Technology into Molecular Medicine and the useful is the application of Genome Wide Studies. *Pakistan Journal of Medical & Health Sciences*, 16(10), 217–220. <https://doi.org/10.53350/pjmhs221610217>
29. Khatoon, F. (2022, August 30). Association of Genetic and Reproductive Hormone with Infertility in Male. *Progress in Medical Sciences*, 1–11. [https://doi.org/10.47363/pms/2022\(6\)175](https://doi.org/10.47363/pms/2022(6)175)
30. Kausar, M. A., Shahid, S., Anwar, S., Kuddus, M., Khan, M. K. A., Khalifa, A. M., Khatoon, F., Alotaibi, A. D., Alkhodairy, S. F., Snoussi, M., & Arif, J. M. (2022, February 4). Identifying the alpha-glucosidase inhibitory potential of dietary phytochemicals against diabetes mellitus type 2 via molecular interactions and dynamics simulation. *Cellular and Molecular Biology*, 67(5), 16–26. <https://doi.org/10.14715/cmb/2021.67.5.3>
31. Zahid Balouch FK, editor. *Therapeutic Proteins Against Human Diseases* [Internet]. Springer Nature Singapore; 2022. Available from: <http://dx.doi.org/10.1007/978-981-16-7897-4i.org/10.14715/cmb/2021.67.5.3>
32. Khatoon, F. (2022, August 30). Association of Genetic and Reproductive Hormone with Infertility in Male. *Progress in Medical Sciences*, 1–11. [https://doi.org/10.47363/pms/2022\(6\)175](https://doi.org/10.47363/pms/2022(6)175)
33. Kausar, M. A., Shahid, S., Anwar, S., Kuddus, M., Khan, M. K. A., Khalifa, A. M., Khatoon, F., Alotaibi, A. D., Alkhodairy, S. F., Snoussi, M., & Arif, J. M. (2022, February 4). Identifying the alpha-glucosidase inhibitory potential of dietary phytochemicals against diabetes mellitus type 2 via molecular interactions and dynamics simulation. *Cellular and Molecular Biology*, 67(5), 16–26. <https://doi.org/10.14715/cmb/2021.67.5>
34. Sarwar Beg, Waleed Hassan Almalki, Fahmida Khatoon, Arshi Malik, Sarah Afaq, Hani Choudhry. Lipid- and polymer-based nanocomplexes in nucleic acid delivery as cancer vaccines, *Drug Discovery Today*, 2021, ISSN 1359-6446. <https://doi.org/10.1016/j.drudis.2021.02.013>
35. Kausar, M. A., Anwar, S., Eltayb, W. A., Kuddus, M., Khatoon, F., El-Arabey, A. A., Khalifa, A. M., Rizvi, M. R., Najm, M. Z., Thakur, L., Kar, S., & Abdalla, M. (2022, August 5). MD Simulation Studies for Selective Phytochemicals as Potential Inhibitors against

- Major Biological Targets of Diabetic Nephropathy. *Molecules*, 27(15), 4980. <https://doi.org/10.3390/molecules27154980>
36. Kahtoon, F., Ahmed, R. M. E., Iqbal, N., Balouch, Z., & Alenazi, F. S. (2021). Genetic Identification: A Review on Autosomal Single Nucleotide Polymorphism's as Diagnostic Tool for Identifying Human. *Journal of Pharmaceutical Research International*, 32(46), 25-33. <https://doi.org/10.9734/jpri/2020/v32i4631099>
37. Saleem, M., Kausar, M. A., Khatoon, F., Anwar, S., Shahid, S. M. A., Ginawi, T., Hossain, A., Al Anizy, A. A. S. A., A. Alswaidan, M. A., Saleh Aseeri, A., Saloom Alturjmi, M. H. B., Abdulkarim, D. F., & Kuddus, M. (2020). Association between Human Health and Indoor Air Pollution in Saudi Arabia: Indoor Environmental Quality Survey. *Journal of Pharmaceutical Research International*, 32(34), 57-66. <https://doi.org/10.9734/jpri/2020/v32i3430965>
38. Fahmida K. Recent Techniques Based on the Utilization of DNA and Autosomal Single Nucleotide Polymorphism. *Gomal Journal of Medical Sciences*, Volume 16 April-June 2019 Vol 17, NO 2. Pg 59-62 ;ISSN: 1819-7973 [https://www.pakmedinet.com/journal/53/1/June/2019/17\(2\)](https://www.pakmedinet.com/journal/53/1/June/2019/17(2))
39. Fahmida Khatoon. Recent techniques based on the utilization of DNA and autosomal single nucleotide polymorphisms for identifying humans. *Gomal J Med Sci Apr - Jun 2019*;17(2):58-62 IS
40. Fahmida K .Use of Deoxy ribonucleic Acid in human identification. *Gomal Journal of Medical Sciences*, Volume 16 Oct-Dec 2018 ISSN: 1819-7973 <https://www.pakmedinet.com/43017>